



## Development of an electrochemical sensor to determine amoxicillin in natural water based on CORE-SHELL/PVP

ARTICLES doi:10.4136/ambi-agua.3070

Received: 27 Mar. 2025; Accepted: 07 Jun. 2025

Renata Kelly Mendes<sup>1\*</sup>; Adriana Roberta Candido<sup>1</sup>  
Julia Boiago Ferraz de Oliveira<sup>2</sup>; Wyllerson Evaristo Gomes<sup>1</sup>

<sup>1</sup>Programa de Pós-Graduação em Sistemas de Infraestrutura Urbana. Pontifícia Universidade Católica de Campinas (PUC-Campinas), Rua Professor Doutor Euryclides de Jesus Zerbini, n° 1516, CEP: 13087-571, Campinas, SP, Brazil. E-mail: adrianarobertacandido@gmail.com, pesquisawyll@gmail.com

<sup>2</sup>Faculdade de Química. Pontifícia Universidade Católica de Campinas (PUC-Campinas), Rua Professor Doutor Euryclides de Jesus Zerbini, n° 1516, CEP: 13087-571, Campinas, SP, Brazil.

E-mail: julia.bfo@puccampinas.edu.br

\*Corresponding author. E-mail: renatavalente@puc-campinas.edu.br

Editor-in-Chief: Nelson Wellausen Dias

### ABSTRACT

In 2020, the world was affected by a new virus, SARS-CoV-2, which causes the disease known as COVID-19. Given the damage caused by the pandemic, there was a significant increase in the use of antibiotics. However, this increase causes harmful effects due to disposal in sewage systems by human and animal excretion and their manufacturing process. These drugs reach water resources, causing environmental impacts and damage. Given this current and worrying scenario, the focus of this work was to develop an alternative and lower-cost method for the detection of amoxicillin in natural urban waters, using an electrochemical sensor based on a core-shell formed by Fe<sub>3</sub>O<sub>4</sub>@Ag coated with the polymer polyvinylpyrrolidone. The device presented a wide linear range between 136 and 8210 µmol L<sup>-1</sup> of amoxicillin, with a detection limit of 7.8 µmol L<sup>-1</sup>. When applied to detect the analyte in urban natural water samples and in commercial drugs, it presented a low relative error of 2.7% and 5.1%, respectively. Thus, the device proved to be an excellent alternative for detecting antibiotics in real samples, in addition to being miniaturized, allowing low-cost field analysis.

**Keywords:** amoxicillin, emerging pollutant, Fe<sub>3</sub>O<sub>4</sub>@Ag core-shell.

### Desenvolvimento de um sensor eletroquímico para a determinação de antibióticos em águas naturais baseado em CORE-SHELL/PVP

### RESUMO

Em 2020, o mundo foi afetado por um novo vírus, o SARS-CoV-2, causador da doença conhecida como COVID-19. Diante dos danos causados pela pandemia, houve um aumento significativo no consumo de antibióticos. No entanto, esse aumento causa efeitos nocivos devido ao descarte em sistemas de esgoto por excreção, humana e animal, e seu processo de fabricação. Esses medicamentos atingem os recursos hídricos, causando impactos e danos ambientais. Diante desse cenário atual e preocupante, o foco deste trabalho foi desenvolver um método alternativo e de menor custo para detecção de amoxicilina em águas urbanas naturais,



utilizando um sensor eletroquímico baseado em core-shell formado por  $\text{Fe}_3\text{O}_4@\text{Ag}$  revestido com o polímero polivinilpirrolidona. O dispositivo apresentou uma ampla faixa linear entre 136 e  $8210 \mu\text{mol L}^{-1}$  de amoxicilina, com limite de detecção de  $7,8 \mu\text{mol L}^{-1}$ . Quando aplicado para detectar o analito em amostras de águas naturais urbanas e em medicamentos comerciais, apresentou baixo erro relativo de 2,7% e 5,1%, respectivamente. Dessa forma, o dispositivo se mostrou uma excelente alternativa para detecção de antibióticos em amostras reais, além de ser miniaturizado, permitindo análises de campo de baixo custo.

**Palavras-chave:** amoxicilina, core-shell de  $\text{Fe}_3\text{O}_4@\text{Ag}$ , poluentes emergentes.

## 1. INTRODUCTION

The world has recently experienced the tragic and historic COVID-19 pandemic, a disease caused by the SARS-COV-2 virus, popularly known as coronavirus. In March 2020, after several cases and worldwide alerts, COVID-19 was characterized by the World Health Organization (WHO) as a pandemic (Buss *et al.*, 2020).

One of the consequences caused by the pandemic was the significant increase in the use of antibiotics, used to prevent and treat infections in humans and animals. A study conducted by Rabbi *et al.* (2023), indicated that in 2020 there was a 26% increase in the consumption of these drugs compared to previous years. It is estimated that the rate of bacterial co-infection during the pandemic was below 10%, but antibiotics were prescribed to 75% of patients who were infected by the virus, since there were no medications for specific treatment of the disease at that time (Nandi *et al.*, 2023).

The impacts of the antibiotics' excessive use raise several questions related to public health and environmental issues. In terms of health, the greatest concern is the increase in antibiotic resistance genes, which can promote changes in the microbial community and generate superbugs (Hosseini and Ripanda, 2025). In terms of environmental impacts, the concern is related to the disposal of these compounds in hospital and domestic sewage. According to specific studies, only 15% of antimicrobial products are metabolized by the human body. The remainder can be excreted as active chemical substances (Zhao *et al.*, 2023).

Among the antibiotics prescribed, amoxicillin ( $\text{C}_{16}\text{H}_{19}\text{N}_3\text{O}_5\text{S}$ ) has a prominent role because it is easily accessible, with broad bactericidal spectrum and has a proven high rate of efficacy, capable of covering wide range of infections in both humans and animals, due to extremely strong bactericidal effect (Chávez *et al.*, 2024; Feroze *et al.*, 2023; Wang and Zhang, 2022). In this way, amoxicillin ( $\text{pK}_{\text{a}1}$  of 2.8 and  $\text{pK}_{\text{a}2}$  of 7.2) is currently considered an emerging pollutant, a compound that can pose risks to the ecosystem and public health causing allergic reactions and liver and kidney dysfunction, but it is not yet regulated. Therefore, there is not enough monitoring data to measure the environmental impact caused (Cartaxo *et al.*, 2020; Li *et al.*, 2020).

Given this real and worrying scenario, it is necessary to develop alternatives for controlling, identifying and detecting these compounds in environmental matrices. Currently, the most widely used methods for determining antibiotics in natural waters are chromatographic methods, such as high-performance liquid chromatography (HPLC) (Hu *et al.*, 2024; Dousa and Hosmanová, 2005) and UPLC (Abdallah *et al.*, 2019). However, it is known that it has high operational costs and requires specific technical training. In this context, the use of electrochemical sensors is relevant, which have been widely applied for chemical pollutants. These devices allow rapid, low-cost, sensitive and highly reliable analyses in complex samples. Oliveira *et al.* (2022) as well as Souza *et al.* (2023) developed an electrochemical sensor based on printed carbon electrodes and titanium dioxide/cobalt composite to determine amoxicillin, presenting a linear region of 20 to  $150 \mu\text{mol L}^{-1}$  and a limit of detection of  $5.8 \mu\text{mol L}^{-1}$ . In

another study, the electrochemical device was constructed using a printed cellulose nanofiber electrode modified with multi-walled carbon nanotubes wrapped in polybenzimidazole, achieving a limit of detection of  $0.3 \mu\text{mol L}^{-1}$  and a wide linear range of 0.3 to  $500 \mu\text{mol L}^{-1}$  (Sari *et al.*, 2023).

Great attention has been given to core-shell nanomaterials, which are composed of nanoparticles denominated as core covered with another nanoparticle as shell (Zibadi *et al.*, 2024). Core-shell structures formed by  $\text{Fe}_3\text{O}_4$  nanoparticles have shown characteristics interesting considering electrochemical sensor development such as excellent conductivity, affordable cost and magnetic properties that facilitate the washing steps, since they are easily attracted by a magnetic field and redispersed in its absence (Li and Wang, 2024). To improve the stability of this nanomaterial, they can be coated with nanoparticles of noble metals, such as silver. Silver nanoparticles still have low electrical resistance, good conductivity and excellent biocompatibility (Palsaniya *et al.*, 2023).

To avoid the common core-shell agglutination, its coating with polymer is an efficient alternative. Polyvinylpyrrolidone (PVP) is a water-soluble polymer formed by multiple chains of vinyl pyrrolidones and it contains lactam ring as repeating unit in chain, which gives advantageous characteristics such as the ability to form stable complexes (Sophia and Muralidharan, 2015). PVP presents biocompatibility and non-toxicity and the use of PVP in sensors can also improve the mechanical and electrical properties of the devices (Pourmadadi *et al.*, 2023).


In this context, the aim of this work is to develop an electrochemical sensor based on a  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell modified with PVP for the determination of the antibiotic amoxicillin in natural urban waters.

## 2. MATERIAL AND METHODS

Ammonia,  $\text{FeCl}_2$ ,  $\text{FeCl}_3$ ,  $\text{AgNO}_3$  and PVP (PA) was obtained from Synth (Brazil). Amoxicillin (PA) and other reagents (analytical grade) were purchased from Sigma-Aldrich. Phosphate buffer solutions were obtained by mixing solutions of  $0.1 \text{ mol L}^{-1}$   $\text{Na}_2\text{HPO}_4$  and  $0.1 \text{ mol L}^{-1}$   $\text{NaH}_2\text{PO}_4$  in ultrapure water. All solutions were prepared with deionized water ( $> 18 \text{ M}\Omega \text{ cm}$ , Milli-Q, Millipore).

### 2.1. $\text{Fe}_3\text{O}_4@\text{Ag}$ Core-shell preparation

The core-shell synthesis followed the procedure adapted from Ahrberg *et al.* (2020). For the preparation, a flow-through system (FIA) was used, which allows the continuous addition of aqueous solutions of the reagents. For this purpose, a multichannel peristaltic pump was used to inject in a flow at a rate of  $1.0 \text{ mL minute}^{-1}$ ,  $4 \text{ mol L}^{-1}$  ammonia solution (channel 1), mineral oil (Nujol) with surfactant additive Triton-X 100 0.075% and Tween-80 1.75% (channel 2) and in the third channel a mixture of  $\text{FeCl}_2$  solution  $0.03 \text{ mol L}^{-1}$  and  $\text{FeCl}_3$   $0.06 \text{ mol L}^{-1}$ , as shown in Figure 1. The solution was mixed in a tap with input from 3 channels and output to the thermostatic bath at a temperature of  $70^\circ\text{C}$ , where the solution circulated for 10 minutes. Then,  $0.03 \text{ mol L}^{-1}$  silver nitrate was added to channel 4 and the system began to produce the core-shell continuously.

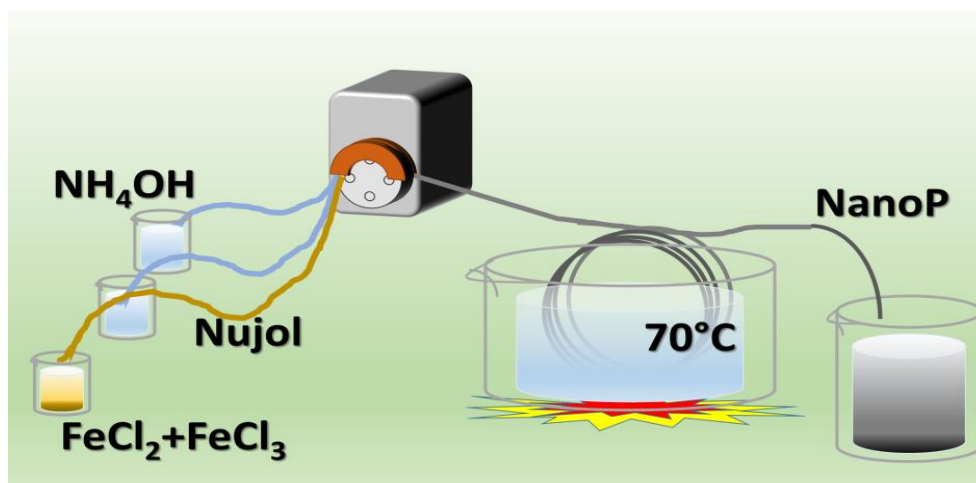

**Figure 1.** Schematic of the assembly for the synthesis of  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell in a flux system.

## 2.2. Sensor Construction

To recover the nanostructure with the polymer, 50  $\mu\text{L}$  of the core-shell solution and 50  $\mu\text{L}$  of the 100  $\text{mg L}^{-1}$  PVP solution were added to an Eppendorf<sup>®</sup> flask and left to interact for 60 min. Afterwards, the system was washed with 0.1  $\text{mol L}^{-1}$  phosphate buffer solution to remove the weakly adsorbed polymer. So, 5  $\mu\text{L}$  of the core-shell/PVP was dripped on a graphite screen-printed electrode from Metrohm<sup>®</sup>, with dimensions of 3.4 x 1.0 x 0.05 cm. After drying the drop, it was used as a sensor for amoxicillin.

## 2.3. Electrochemical Measurements

The measurements with 300  $\text{mg L}^{-1}$  amoxicillin were carried out using differential pulse voltammetry technique, in the range of -200 to 1000 mV with 25 mV amplitude at 50  $\text{mV s}^{-1}$ . All experiments were carried out in an AUTOLAB micro potentiostat (Metrohm) PGSTAT 204.

## 2.4. Scanning Electron Microscopy (SEM) Imaging


The SEM imaging was performed in the JEOL equipment - Model JSM IT500HR. The image captures of the compounds were randomly selected in fields in the samples and at three magnifications: 10,000X, 20,000X and 30,000X. The preparation consisted in drying the solvent, from the samples suspended in aqueous medium, which were deposited on a glass slide and left in atmospheric air for 24 hours.

# 3. RESULTS AND DISCUSSION

## 3.1. Core-shell Characterization


Before applying the proposed sensor, it was necessary to characterize the core-shell to verify it was produced efficiently. Figure 2 shows the ultraviolet-visible (UV) spectra obtained for both the  $\text{Fe}_3\text{O}_4$  nanoparticle (2A) and after its coating with silver nanoparticles to form the core-shell (2B), after dilution in deionized water (1:100).

Analysing Figure 2, it is possible to observe that for  $\text{Fe}_3\text{O}_4$  nanoparticles there are two absorption bands, at 250 and 350 nm, which coincides with that obtained by Ramesh *et al.* (2017). For core-shell, it is verified that the absorption at 350 nm is maintained (referring to iron oxide) and there is the appearance of a band at 487 nm (highlight on Figure 2B) which refers to the resonance plasmons of silver, as described by Nana Kaka *et al.* (2023). Based on this analysis, it is possible to confirm the formation of the core-shell product  $\text{Fe}_3\text{O}_4@\text{Ag}$ .

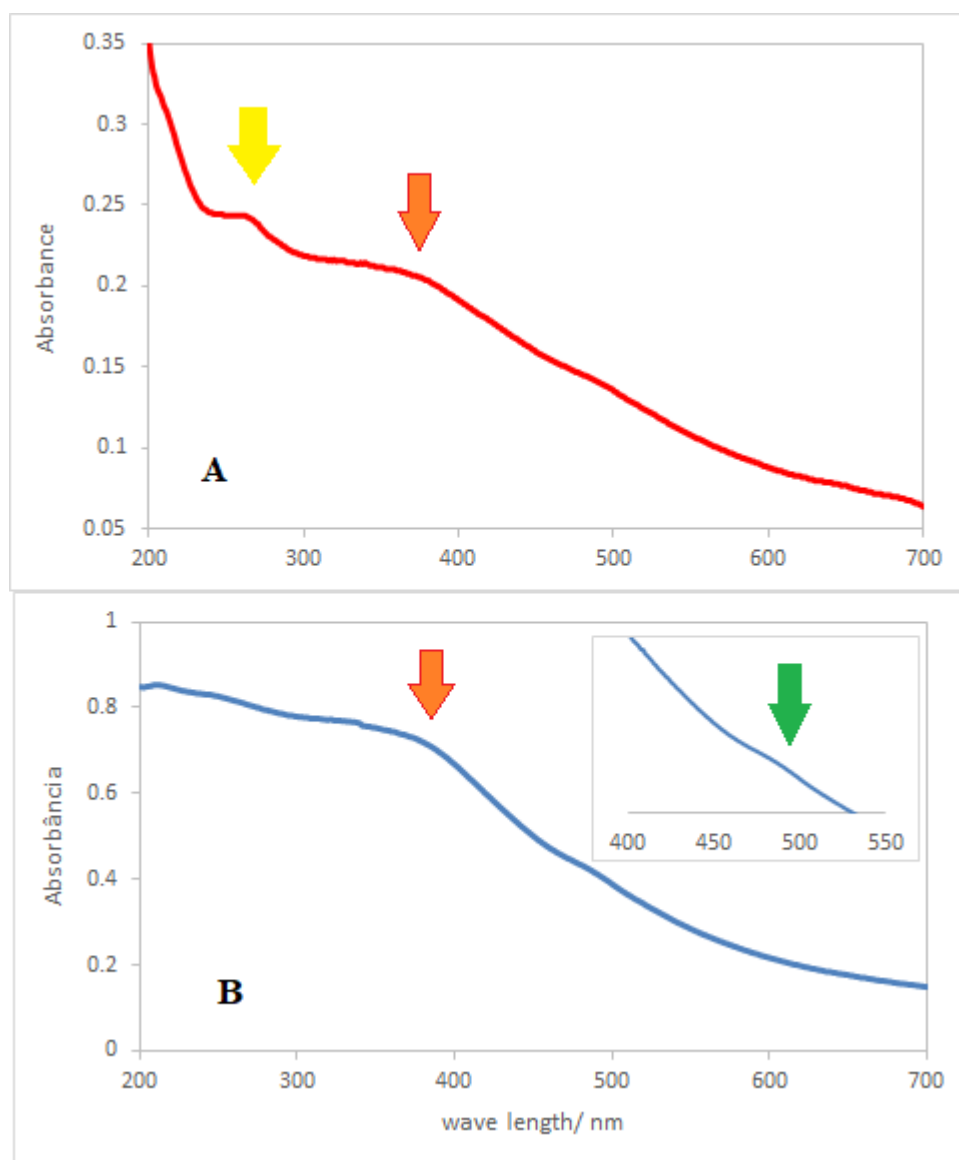

**Figure 2.** UV-Vis spectra obtained for Fe<sub>3</sub>O<sub>4</sub> nanoparticles (A) and for the Fe<sub>3</sub>O<sub>4</sub>@Ag core-shell (B).

After spectroscopic characterization of the core-shell, images were obtained using scanning electron microscopy (SEM), aiming to estimate the morphology of the nanomaterial. The following were analyzed: (I) the pure Fe<sub>3</sub>O<sub>4</sub> nanoparticles; (II) the Fe<sub>3</sub>O<sub>4</sub>@Ag core-shell and (III) the core-shell after coating with PVP. Figure 3 shows the results obtained, respectively.

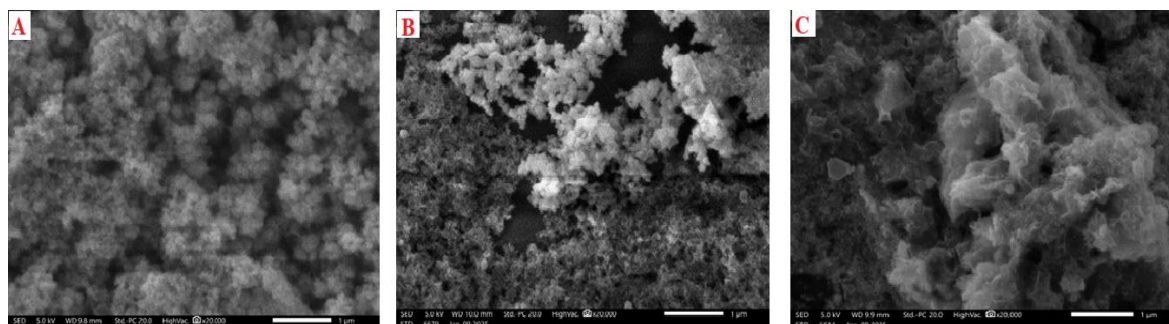


**Figure 3.** SEM images of the Fe<sub>3</sub>O<sub>4</sub> nanoparticles (A); Fe<sub>3</sub>O<sub>4</sub>@Ag core-shell nanostructure (B) and Fe<sub>3</sub>O<sub>4</sub>@Ag/PVP nanocomposite (C) 20,000 times magnification.

Observing Figures 3, it is possible to verify different morphologies among the analyzed samples. It was not possible to perform measurements for the nanoparticle size, due to restrictions on the equipment and because of conditions of agglomeration and coating by other compounds.

In Figure 3A, aspects of nanoparticle clusters are observed throughout the sample field. These nanoparticles have spherical shapes and a high density of the nanomaterial is observed, showing the tendency to agglomeration. In Figure 3B, vacancies are noted in the sample field, indicating a tendency to deagglomeration in relation to the pure nanoparticles, which was already expected by the addition of silver. A certain increase in the nanostructures size was observed when comparing the images A and B. It also increased brightness in the images, establishing the silver coating. In Figure 3C, a film covering the material is noticeable which was not present in the previous images. The size of nanocomposite is larger than observed in the core-shell.

To verify the influence of the core-shell coating by PVP on the electrochemical measurements, measurements with  $136 \mu\text{mol L}^{-1}$  amoxicillin solution were performed using differential pulse voltammetry (DPV) under the following conditions: (I) the pure  $\text{Fe}_3\text{O}_4$  nanoparticles; (II) the  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell; (III) the core-shell after coating with PVP and (IV) the core-shell after coating with PVP in  $0.1 \text{ mol L}^{-1}$  phosphate buffer solution. Figure 4 presents the results obtained.

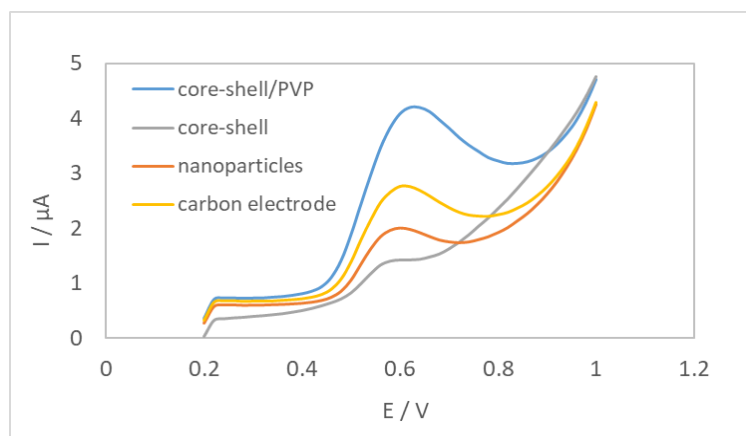

**Figure 4.** Differential Pulse Voltammograms of the  $\text{Fe}_3\text{O}_4$  nanoparticles (A);  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell nanostructure (B)  $\text{Fe}_3\text{O}_4@\text{Ag}/\text{PVP}$  nanocomposite (C) in  $136 \mu\text{mol L}^{-1}$  amoxicillin solution in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7.0 and  $\text{Fe}_3\text{O}_4@\text{Ag}/\text{PVP}$  nanocomposite in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7. Pulse amplitude was 25 mV, at  $50 \text{ mV s}^{-1}$ .

A peak near 0.6 V shown in the voltammogram is due to the oxidation of hydroxyl (phenolic group) in carbonyl (ketone) in the amoxicillin molecule (Aihaiti *et al.*, 2021). Observing the voltammograms, it is possible to verify that the electrode modified with  $\text{Fe}_3\text{O}_4$  nanoparticles provides a significant signal for the antibiotic since nanomaterials tend to improve electron transfer processes Prakash *et al.* (2013). When the core-shell was tested an increase in the signal was observed. This is because silver nanoparticles have catalytic properties, in addition to high electrical conductivity, which are advantageous in the development of electrochemical devices, contributing to an increase in the response (Huang *et al.*, 2014). With the addition of PVP, an increase in the electrochemical signal was observed because it prevents the nanoparticles agglomeration. Furthermore, it is highlighted that PVP covers the core-shell by hydrophobic bonds between polymer and the Ag nanoparticle (Garcia *et al.*, 2023). The response is not observed when the proposed sensor is evaluated in phosphate buffer solution

(4D). Table 1 presents the current values obtained.

**Table 1.** Current values obtained by DPV voltammograms for different configurations of devices in  $136 \mu\text{mol L}^{-1}$  amoxicillin solution in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7.0.

| Configuration                                | I / $\mu\text{A}$ |
|----------------------------------------------|-------------------|
| Carbon printed electrode                     | 1.4               |
| $\text{Fe}_3\text{O}_4$ nanoparticle         | 2.0               |
| $\text{Fe}_3\text{O}_4@\text{Ag}$            | 2.8               |
| $\text{Fe}_3\text{O}_4@\text{Ag}/\text{PVP}$ | 4.2               |

Based on the data obtained by UV-Vis spectroscopy, SEM images and DPV measurements, we can confirm the satisfactory production of the core-shell as well as its subsequent coating by the polymer. Thus, the proposed architecture for the amoxicillin sensor proved to be very efficient and, therefore, the study of the optimization of the experimental conditions was followed.

### 3.2. Experimental Conditions Optimization

Before applying the proposed sensor to real samples, a crucial step is required to select the best experimental conditions. This allows us to increase the sensitivity of the device, since the conditions in which its response is maximum will be selected.


Firstly, studies were carried out involving the selection of the polymer to cover the core-shell: Polyvinylpyrrolidone (PVP), Diethanolamine and Chitosan. Then, differential pulse voltammograms were obtained in  $820 \mu\text{mol L}^{-1}$  antibiotic solution in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7.0. Each polymer covers the core-shell for 30 min. The best response was obtained when PVP was used (data in Supplementary Material). Studies show that PVP helps maintain the colloidal shape of the nanomaterial, preventing it from undergoing aggregation processes, which could impair the signal (Pourmadadi *et al.*, 2023). Chitosan was the material that presented the lowest response, probably due to its terminal  $-\text{NH}_2$  groups that did not contribute to the interaction with the analyte. Thus, PVP was used in subsequent experiments.

Another study is the most suitable PVP concentration for coating the  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell. DPV measurements were carried out on the device containing three different concentrations of the polymer: 100; 500 and  $1000 \text{ mg L}^{-1}$ . It was concluded that the best concentration to be used is  $100 \text{ mg L}^{-1}$  (data in Supplementary Material) due to larger polymer concentration to lead to decrease in the response. This is probably because there is an increase in the thickness of the polymeric layer with larger concentration, which can hinder the transfer of electrons, leading to a decrease in the electrochemical signal (Wang *et al.*, 2023).

The latest study carried out refers to the interaction time between PVP and core-shell. The times evaluated were: 15, 30, 45 and 60 minutes. Analyzing the results obtained (data in Supplementary Material), increasing the interaction time increases the signal. Longer times were not tested as they would not be appropriate for sensor assembly, especially considering more quickly in the construction, since the proposal is that it should be easy to use, prepare and to be applied in field analyses. Therefore, 60 min was selected for subsequent studies.

### 3.3. Analytical Curve

After optimization, the analytical performance of the proposed sensor was obtained with different concentrations of amoxicillin. Measurements were performed using differential pulse voltammetry with an amplitude of  $25 \text{ mV}$  at a scan rate of  $50 \text{ mV s}^{-1}$ . The voltammograms (A) and linear response by a calibration curve (B) are presented in Figure 5.

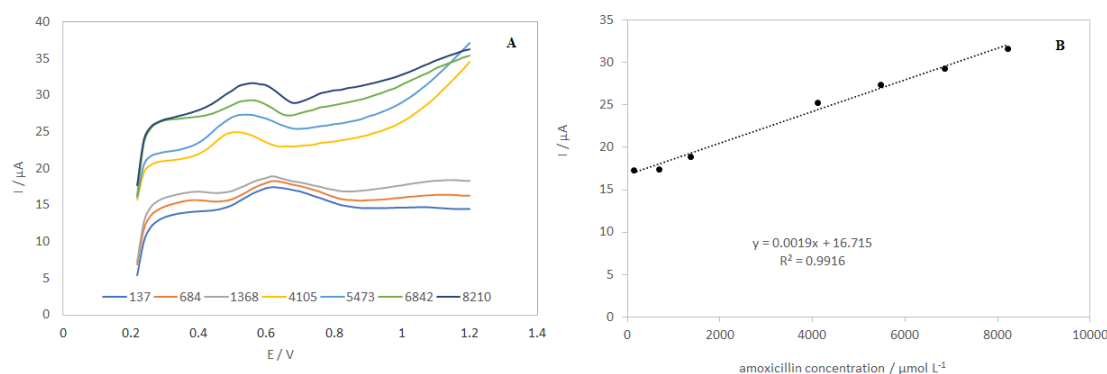

**Figure 5.** DPV (A) and calibration curve (B) of the proposed sensor at different concentrations of amoxicillin in 0.1 mol L<sup>-1</sup> phosphate buffer, pH 7.0. The pulse amplitude was 25 mV, at 50 mV s<sup>-1</sup>.

The analytical curve presents a linear range between 136 to 8210 μmol L<sup>-1</sup> for amoxicillin with the straight-line equation  $y(\mu\text{A}) = 0.0019x(\mu\text{mol L}^{-1}) + 16.715$  ( $R^2 = 0.9916$ ,  $n=7$ ). From the analytical curve, it was calculated the limit of detection (LOD) of 7.8 μmol L<sup>-1</sup> and a limit of quantification (LOQ) of 26.5 μmol L<sup>-1</sup>, using 3.3 Sd/b for LOD and 10 Sd/b for LOQ, being standard deviation of 10 blank measurements (Sd) and the angular coefficient of curve (b).

Analyzing Table 2 is possible to verify that the proposed sensor presents similar magnitudes of linear range when compared with other results in the literature. Furthermore, the proposed sensor is very simple to construct and has a low cost, since the material used as support is very easy to prepare and uses commonly found reagents.

**Table 2.** Proposed sensor characteristics.

| Sensor                                                                                                 | Linear Range /<br>mol L <sup>-1</sup> | Limit of Detection /<br>mol L <sup>-1</sup> | Ref                          |
|--------------------------------------------------------------------------------------------------------|---------------------------------------|---------------------------------------------|------------------------------|
| reduced graphene oxide molecular imprinted overoxidized polypyrrole modified with gold nanoparticles   | 10 <sup>-8</sup> to 10 <sup>-3</sup>  | 1.22 10 <sup>-6</sup>                       | Essousi <i>et al.</i> (2020) |
| glassy carbon electrode modified with reduced graphene oxide and Nafion bismuth selenide nanoparticles | 1.8–5.4 10 <sup>-6</sup>              | 0.36 10 <sup>-6</sup>                       | Valenga <i>et al.</i> (2020) |
| modified reduced graphene oxide over molecular imprinted polymer                                       | 1.42–1100 10 <sup>-6</sup>            | 0.43 10 <sup>-6</sup>                       | Ali and El-Wakil (2023)      |
| reduced graphite oxide nanosheet electrode                                                             | 0.5–80 10 <sup>-6</sup>               | 0.193 10 <sup>-6</sup>                      | Pham <i>et al.</i> (2021)    |
| ZnO semiconductor nanoparticles on graphite carbon sheets                                              | 10 <sup>-4</sup> to 10 <sup>-6</sup>  | 0.121 10 <sup>-6</sup>                      | Zoubir <i>et al.</i> (2021)  |
| Fe <sub>3</sub> O <sub>4</sub> @Ag/PVP on carbon printed electrode                                     | 136–8210 10 <sup>-6</sup>             | 7.8 10 <sup>-6</sup>                        | This work                    |

### 3.4. Determination of Amoxicillin from Commercial Tablet

To verify the efficiency of the sensor in a real sample, it was tested in a commercial drug containing 500 mg of amoxicillin and 125 mg of potassium clavulanate. For the measurements, the tablet was macerated, 8 mg were diluted in a solution containing phosphate buffer pH 7.0 and methanol in a 10 mL flask. Considering the total mass of the tablet was 1.104 g, the expected amoxicillin concentration was 985 μmol L<sup>-1</sup>. The measurements were performed in triplicate and the currents obtained were: 18.90; 18.32 and 18.24 μA. Substituting the average (18.49 μA) into the straight-line equation, the value found was 934 μmol L<sup>-1</sup>. Thus, the relative error was 5.1%, considered excellent, since the medication contained clavulanate in its

composition and excipients. It was verified that the other substances did not interfere significantly in the signal.

### 3.5. Determination of Amoxicillin in Natural Water

To verify the effectiveness of the sensor in a real sample, it was tested with a natural water sample from a lake located Campinas city, at Sao Paulo (Brazil). For the measurements, the natural water was fortified with 300  $\mu\text{mol L}^{-1}$  of amoxicillin. The DPV measurements were performed using five measurements using different sensors constructed in the same conditions (one of the voltammograms in Supplementary Material). The maximum currents obtained were 17.41; 18.03 and 16.50  $\mu\text{A}$ , whose average value was 17.30  $\mu\text{A}$ . Substituting into the straight-line equation, 308  $\mu\text{mol L}^{-1}$  is obtained. Thus, the relative error was 2.67%, considered excellent, since the lake water could contain other interfering substances. Thus, it is verified that the other substances did not interfere with the signal.

## 4. CONCLUSION

According to the results obtained in this work, it is possible conclude that the proposed sensor constructed by core-shell architecture of  $\text{Fe}_3\text{O}_4@\text{Ag}$  coated with polyvinylpyrrolidone (PVP) polymer, proved to be efficient for the detection and quantification of the antibiotic amoxicillin. The device presented satisfactory responses, with a low detection limit of 7.8  $\mu\text{mol L}^{-1}$ , presenting a linear range between 136 and 8210  $\mu\text{mol L}^{-1}$ . When applied to detect the presence of amoxicillin in natural water samples, it presented a low relative error of 2.7%, and in commercial drug samples, the error was 5.1%. Thus, it is proven that other substances present in the water or the tablet do not significantly interfere with the signal. In view of these facts, the miniaturized, low-cost, portable device can be used as a viable alternative for detecting antibiotics in real samples. These contaminants are not eliminated from water by traditional treatment methods, remaining in the matrix, even in low concentrations. The consumption of antibiotics is a concern due to bacterial resistance, which can cause harmful effects on society, including death, especially in urban areas.

## 5. ACKNOWLEDGMENTS

This study was financed in part by the Coordenação de Aperfeiçoamento de Pessoal de Nível Superior - Brazil (CAPES) - Finance Code 001. – scholarship PNPd (Gomes, W.E.) and scholarship PROSUC (Candido, A.R.). Scholarship was financed by FAPESP n. 2024/14003-6 (Oliveira, J.B.F.).

## 6. REFERENCES

- ABDALLAHA, M. A-E.; NGUYEN, K.-H.; EBELE, A. J.; ATIA, N. N.; ALI, H. R. H.; HARRAD, S. A single run, rapid polarity switching method for determination of 30 pharmaceuticals and personal care products in waste water using Q-Exactive Orbitrap high resolution accurate mass spectrometry. **Journal of Chromatography A**, v. 1588, p. 68-76, 2019. <https://doi.org/10.1016/j.chroma.2018.12.033>
- AHRBERG, C.D.; CHOI, J.W.; CHUNG, B. G. Automated droplet reactor for the synthesis of iron oxide/gold core-shell nanoparticles, **Scientific Reports**, v. 10, p. 1737-1745, 2020. <https://doi.org/10.1038/s41598-020-58580-9>

- ALI, R.; EL-WEKIL, M.M. Construction of MIP/Bi<sub>2</sub>S<sub>3</sub> nanoparticles/rGO nanoprobe for simultaneous electrochemical determination of amoxicillin and clavulanic acid. **Journal of Alloys and Compounds**, v. 962, p. 171180, 2023. <https://doi.org/10.1016/j.jallcom.2023.171180>
- AIHAITI, A.; LI, Z.; QIN, Y.; MENG, F.; LI, X.; HUANGFU, Z. *et al.* Construction of electrochemical sensors for antibiotic detection based on carbon nanocomposites. **Nanomaterials**, v. 12, p. 2789, 2021. <https://doi.org/10.3390/nano12162789>
- BUSS, P. M.; ALCÁZAR, S.; GALVÃO, L. A. Pandemia pela Covid-19 e multilateralismo: reflexões a meio do caminho. **Estudos Avançados**, v. 34, n. 99, p. 45-64, 2020. <https://doi.org/10.1590/s0103-4014.2020.3499.004>
- CARTAXO, A. S. B.; ALBUQUERQUE, M. V. C.; SILVA, M. C. C. P.; RODRIGUES, R. M. M.; RAMOS, R. O.; SÁTIRO, J. R. *et al.* Emerging contaminants in waters intended for human consumption: occurrence, implications and treatment technologies. **Brazilian Journal of Development**, v. 6, n. 8, p. 61814–61827, 2020. <https://doi.org/10.34117/bjdv6n8-559>
- CHÁVEZ, C. E. E.; MORA, V. I. C.; BURBANO, K. L. A. Principales antibióticos que generan resistencia antimicrobiana utilizados en procesos odontológicos. Revisión sistemática. **Dominio De Las Ciencias**, v. 10, n. 1, p. 1253-1270, 2024. <https://doi.org/10.23857/dc.v10i1.3773>
- DOUSA, M.; HOSMANOVÁ, R. Rapid determination of amoxicillin in premixes by HPLC. **Journal of Pharmaceutical and Biomedical Analysis**, v. 37, p. 373–377, 2005. <https://doi.org/10.1016/j.jpba.2004.10.010>
- ESSOUSI, H.; BARHOUMI, H.; KARASTOGIANNI, S.; GIROUSI, S.T. An Electrochemical sensor based on reduced graphene oxide, gold nanoparticles and molecular imprinted over-oxidized polypyrrole for amoxicillin determination. **Electroanalysis**, v. 32, p. 1546-1558, 2020. <https://doi.org/10.1002/elan.201900751>
- FEROZE, M. T.; DOONYAPISUT, D.; KIM, B.; CHUNG, C.-H. Impedimetric sensing platform based on copper oxide with activated carbon for sensitive detection of amoxicillin. **Korean Journal of Chemical Engineering**, v. 40, n. 4, p. 1014–1022, 2023. <https://doi.org/10.1007/s11814-022-1366-y>
- GARCIA, S.; MABARROH, N.; DARMAWAN, M. Y.; WIBOWO, N. A.; ARDIYANTI, H.; TUMBELAKA, R. M. *et al.* Two spin-valve GMR thin films on half wheatstone bridge circuit for detecting green-synthesized Fe<sub>3</sub>O<sub>4</sub>@Ag nanoparticles-labeled biomolecule. **Materialia**, v. 32, p. 2-11, 2023. <https://doi.org/10.1016/j.mtla.2023.101930>
- HOSSEIN, M.; RIPANDA, A. S. Pollution by antimicrobials and antibiotic resistance genes in East Africa: Occurrence, sources, and potential environmental implications. **Toxicology Reports**, v. 14, p. 101969, 2025. <https://doi.org/10.1016/j.toxrep.2025.101969>
- HU, J.; BA, Y.; PAN, Z.; LI, X. Simultaneous determination of 50 antibiotic residues in plasma by HPLC–MS/MS. **Heliyon**, v. 10, p. e40629, 2024. <https://doi.org/10.1016/j.heliyon.2024.e40629>

- HUANG, K.-J.; LIU, Y.-J.; WANG, H.-B.; WANG, Y.-Y. A sensitive electrochemical DNA biosensor based on silver nanoparticles-polydopamine@graphene composite. **Electrochimica Acta**, v. 118, p. 130–137, 2014. <http://dx.doi.org/10.1016/j.electacta.2013.12.019>
- LI, B.; WANG, P. Development of a highly sensitive electrochemical sensor for dexamethasone detection using Fe<sub>3</sub>O<sub>4</sub>/polyaniline-Cu(II) microspheres and hematite nanoparticles. **International Journal of Electrochemical Science**, v. 19, p. 100622, 2024. <https://doi.org/10.1016/j.ijoes.2024.100622>
- LI, S.; MA, X.; PANG, C.; LI, H.; LIU, C.; XU, Z. *et al.* Novel molecularly imprinted amoxicillin sensor based on a dual recognition and dual detection strategy. **Analytica Chimica Acta**, v. 1127, p. 69-78, 2020. <https://doi.org/10.1016/j.aca.2020.06.034>
- NANA KAKA, M.; BORAH, N.; GUHA, A. K.; TAMULY, C. Synthesis and characterization of GA-AgNPs for highly sensitive and selective dual colorimetric detection of thiourea and thiophenol with DFT approach. **Inorganic Chemistry Communications**, v. 153, p. 2-11, 2023. <http://doi.org/10.1016/j.inoche.2023.110868>
- NANDI, A.; PECETTA, S.; BLOOM, D. E. Global antibiotic use during the COVID-19 pandemic: analysis of pharmaceutical sales data from 71 countries, 2020–2022. **eClinicalMedicine**, v. 57, p. 101848, 2023. <https://doi.org/10.1016/j.eclinm.2023.101848>
- OLIVEIRA, V. C.; REZENDE, A. A. A.; CALÁBRIA, L. K. Sensores eletroquímicos na detecção de pesticidas em amostras ambientais: uma revisão bibliográfica. **Exatas & Engenharias**, v. 12, n. 35, p. 12–21, 2022. <https://doi.org/10.25242/885x123520222497>
- PALSANIYA, S.; PAL, T.; MUKHERJI, S. Highly sensitive detection of amoxicillin by polyaniline-AgBr amperometry sensor: Fabrication and application in tap water and lake water. **Chemical Engineering Journal**, v. 466, p. 2–12, 2023. <https://doi.org/10.1016/j.cej.2023.143025>
- PHAM, T. H. Y.; MAI, T. T.; NGUYEN, H. A.; CHU, T. T. H.; VU, T. T. H.; LE, Q. H. Voltammetric determination of amoxicillin using a reduced graphite oxide nanosheet electrode. **Journal of Analytical Methods in Chemistry**, p. 8823452, 2021. <https://doi.org/10.1155/2021/8823452>
- POURMADADI, M.; SHAMSABADIPOUR, A.; ASLANI, A.; ESHAGHI, M. M.; RAHDAR, A.; PANDEY, S. Development of Polyvinylpyrrolidone-Based nanomaterials for biosensors applications: A Review. **Inorganic Chemistry Communications**, v. 152, p. 2-16, 2023. <https://doi.org/10.1016/j.inoche.2023.110714>
- PRAKASH, S.; CHAKRABARTY, T.; SINGH, A. K.; SHAHI, V. K. Polymer thin films embedded with metal nanoparticles for electrochemical biosensors applications. **Biosensors and Bioelectronics**, v. 41, n. 1, p. 43-53, 2013. <http://dx.doi.org/10.1016/j.bios.2012.09.031>
- RABBI, F.; BANFIELD, L.; MUNIR, M.; CHAGLA, Z.; MAYHEW, A.; SOUZA, R. J. Overprescription of antibiotics for treating hospitalized COVID-19 patients: A systematic review & meta-analysis. **Heliyon**, v. 9, n. 10, p. 2-11, 2023. <https://doi.org/10.1016/j.heliyon.2023.e20563>


- RAMESH, A. V. *et al.* A facile plant mediated synthesis of magnetite nanoparticles using aqueous leaf extract of *Ficus Hispida* L. for adsorption of organic dye. **IOSR Journal of Applied Chemistry**, v. 10, p. 35-43, 2017. <https://doi.org/10.9790/5736-1007013543>
- SARI, S. R.; SHINCHI, E.; SHIDA, K.; KUSUMAWATI, Y.; MADURANI, K. A.; KURNIAWAN, F. *et al.* A green cellulose nanofiber-based printed electrode for practical highly sensitive amoxicillin detection. **Analyst**, v. 148, p. 2932-2940, 2023. <https://doi.org/10.1039/D3AN00453H>
- SOPHIA, J.; MURALIDHARAN, G. Polyvinylpyrrolidone stabilized palladium nanospheres as simple and novel electrochemical sensor for amperometric hydrogen peroxide detection. **Journal of Electroanalytical Chemistry**, v. 739, p. 115-121, 2015. <https://doi.org/10.1016/j.jelechem.2014.12.021>
- SOUZA, L. K. A.; SILVA-NETO, H. A.; ROCHA, D. S.; ABREU, F. C.; SILVA, A. C. A.; DANTAS, N. O. *et al.* Disposable sensor based on carbon electrodes modified with cobalt-doped titanium dioxide nanocrystals for electrochemical detection of amoxicillin. **Journal of Electroanalytical Chemistry**, v. 942, p. 2-10, 2023. <https://doi.org/10.1016/j.jelechem.2023.117587>
- VALENGA, M. G. P.; FELSNER, M. L.; MATOS, C. F.; CASTRO, E. G.; GALLI, A. Development and validation of voltammetric method for determination of amoxicillin in river water. **Analytica Chimica Acta**, v. 1138, p. 79-88, 2020. <https://doi.org/10.1016/j.aca.2020.09.020>
- WANG, X.; WANG, R.; XUE, Q.; LIU, Z.; LIU, Y.; WANG, J. *et al.* Detection of cadmium (II) ion in water by a novel electrochemical sensor based on modification of graphite carbon nitride and polyaniline composite. **Diamond and Related Materials**, v. 140, p. 2-9, 2023. <https://doi.org/10.1016/j.diamond.2023.110427>
- WANG, Y.; ZHANG, L. High sensitive label-free electrochemical sensor using polydopamine-coated Zr-MOF composites for rapid detection of amoxicillin. **International Journal of Electrochemical Science**, v. 17, p. 221293, 2022. <https://doi.org/10.20964/2022.12.85>
- ZHAO, L.; LV, Z.; LIN, L.; LI, X.; XU, J.; HUANG, S. *et al.* Impact of COVID-19 pandemic on profiles of antibiotic-resistant genes and bacteria in hospital wastewater. **Environmental Pollution**, v. 334, p. 2-10, 2023. <https://doi.org/10.1016/j.envpol.2023.122133>
- ZIBADI, F.; ZIBADI, F.; REZAYI, M.; OSKUEE, R. K.; BOLOURINEZHAD, M.; DARROUDI, M. *et al.* Designing and evaluation of a novel electrochemical biosensor based on carbon quantum dots and gold core-shell to detect and measure Human T-lymphotropic Virus-1 (HTLV-1) in clinical samples. **Microchemical Journal**, v. 201, p. 110563, 2024. <https://doi.org/10.1016/j.microc.2024.110563>
- ZOUBIR, J.; IDRIS, B.; ALI, A. Synthesis of ZnO nanoparticles on carbon graphite and its application as a highly efficient electrochemical nano-sensor for the detection of amoxicillin: analytical application: milk, human urine, and tap water. **Nanotechnology for Environmental Engineering**, v. 6, p. 54-74, 2021. <https://doi.org/10.1007/s41204-021-00146-9>

## Supplementary Data

### 1. Optimization of experimental conditions

Before applying the proposed sensor to real samples, a very important step is required to select the best experimental conditions. This allows us to increase the sensitivity of the device, since the conditions in which its response is maximum will be selected.

Firstly, studies were carried out involving the selection of the polymer to cover the core-shell: Polyvinylpyrrolidone (PVP), Diethanolamine and Chitosan. Then, differential pulse voltammograms were obtained in a  $300 \text{ mg L}^{-1}$  antibiotic solution in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7.0. Each polymer covered the core-shell for 30 min. Figure 1 presents the results.

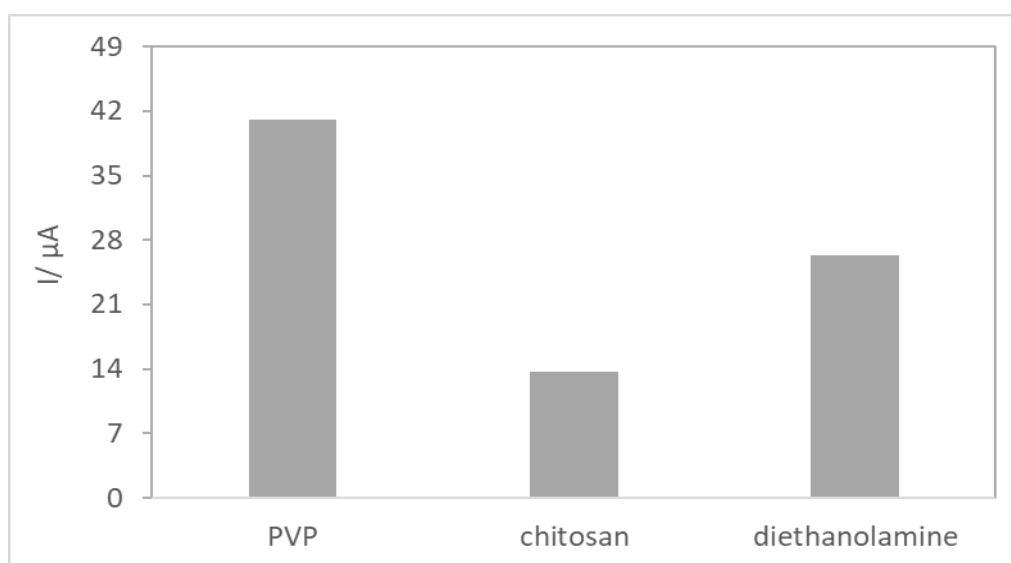


**Figure 1.** Currents obtained for carbon-printed electrodes containing  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell coated with different compounds. In  $300 \text{ mg L}^{-1}$  amoxicillin solution in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7.0. Pulse amplitude was  $25 \text{ mV}$ , at  $50 \text{ mV s}^{-1}$ .

Observing Figure 1, it is possible to verify that the best response was obtained when PVP was used. Studies show that PVP helps maintain the colloidal shape of the nanomaterial, preventing it from undergoing aggregation processes, which could impair the signal (Pourmadadi et al., 2023). Chitosan was the material that presented the lowest response, probably due to its terminal  $-\text{NH}_2$  groups that did not contribute to the interaction with the analyte. Thus, PVP was used in subsequent experiments.


Another study is the most suitable PVP concentration for coating the  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell. DPV measurements were carried out on the device containing three different concentrations of the polymer:  $100$ ;  $500$  and  $1000 \text{ mg L}^{-1}$ . Figure 2 shows the results.

It was concluded that the best concentration to be used is  $100 \text{ mg L}^{-1}$  due to larger polymer concentration that leads to a decrease in the response. This is probably because there is an increase in the thickness of the polymeric layer with larger concentration, which can hinder the transfer of electrons, leading to a decrease in the electrochemical signal (Wang et al., 2023).

The latest study carried out refers to the interaction time between PVP and core-shell. The times evaluated were:  $15$ ,  $30$ ,  $45$  and  $60$  minutes. Analyzing the results (Figure 3), it can be seen that increasing the interaction time increases the signal. Longer times were not tested as they would not be appropriate for biosensor assembly, especially considering more quickly in the construction, since the proposal is that it should be easy to use, prepare and to be applied in field analyses. Therefore, the time of  $60 \text{ min}$  was selected for subsequent studies.

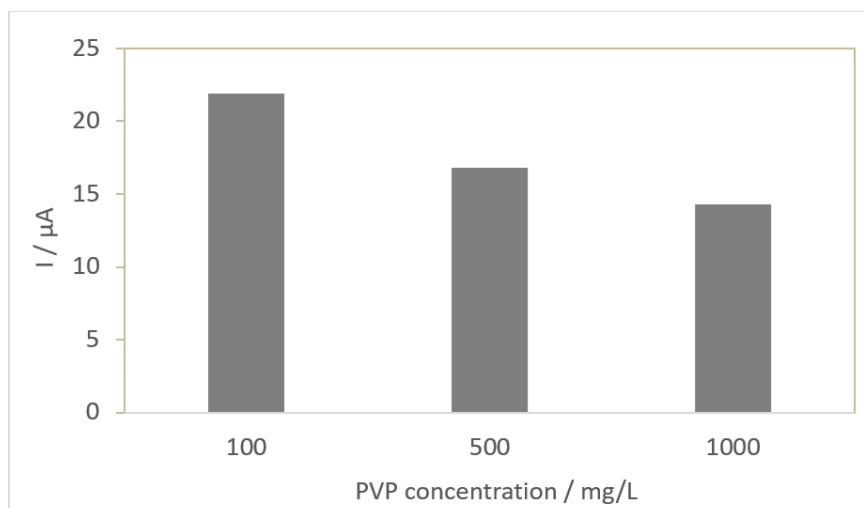


**Figure 2.** Currents obtained for carbon-printed electrodes containing  $\text{Fe}_3\text{O}_4@\text{Ag}$  with different concentrations of PVP. in  $300 \text{ mg L}^{-1}$  amoxicillin solution in  $0.1 \text{ mol.L}^{-1}$  phosphate buffer pH 7.0. Pulse amplitude was 25 mV, at  $50 \text{ mV s}^{-1}$ .

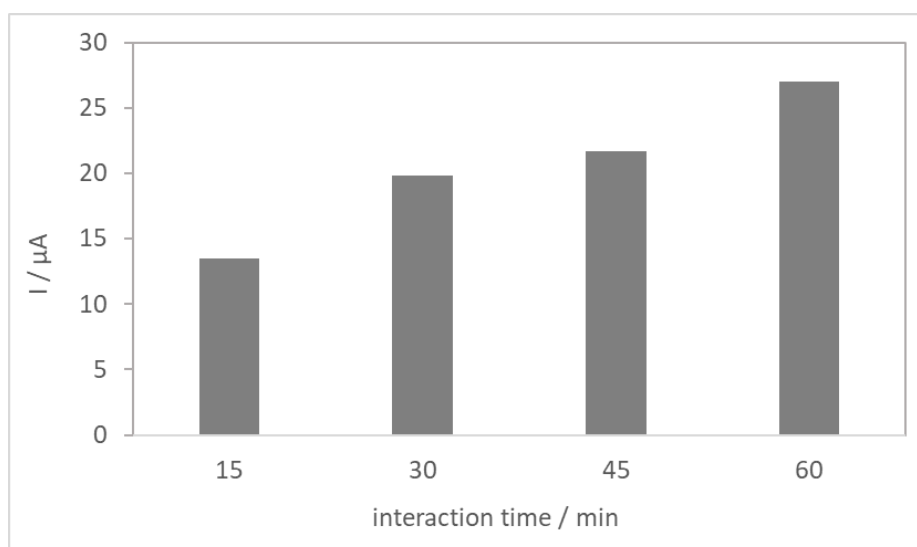

**Figure 3.** Currents obtained in different times of interaction between  $\text{Fe}_3\text{O}_4@\text{Ag}$  core-shell and PVP. in  $300 \text{ mg L}^{-1}$  amoxicillin solution in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7.0. Pulse amplitude was 25 mV, at  $50 \text{ mV s}^{-1}$ .

## 2. Determination of Amoxicillin from Commercial Tablet


To verify the efficiency of the sensor in a real sample, it was tested with a commercial drug containing 500 mg of amoxicillin and 125 mg of potassium clavulanate. For the measurements, the tablet was macerated, 8 mg were diluted in a solution containing phosphate buffer pH 7.0 and methanol in a 10 mL flask. Considering the total mass of the tablet was 1.104 g, the expected amoxicillin concentration was  $985 \mu\text{mol L}^{-1}$ . The measurements were performed in triplicate and the currents obtained were: 18.90; 18.32 and  $18.24 \mu\text{A}$ . Substituting the average ( $18.49 \mu\text{A}$ ) into the straight-line equation, the value found was  $934 \mu\text{mol L}^{-1}$ . Thus, the relative error was 5.1 %, considered excellent, since the medication contained clavulanate in its composition and excipients. It was verified that the other substances did not interfere significantly in the signal. Figure 4 presents the voltammogram obtained.

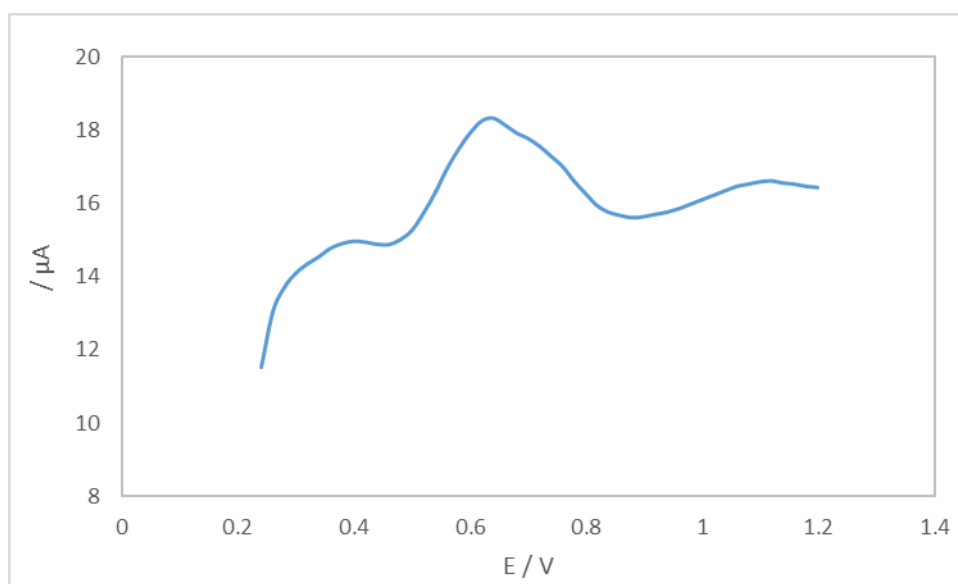

**Figure 4.** Differential Pulse Voltammogram of the sensor in commercial tablet solution in  $0.1 \text{ mol L}^{-1}$  phosphate buffer pH 7.0. Pulse amplitude was 25 mV, at  $50 \text{ mV s}^{-1}$ .

### 3. Determination of Amoxicillin in Natural Water

To verify the effectiveness of the sensor in a real sample, it was tested with a natural water sample from a lake located Campinas city, at Sao Paulo (Brazil). For the measurements, the natural water was fortified with  $300 \text{ } \mu\text{mol L}^{-1}$  of amoxicillin. The DPV measurements were performed using five measurements using different sensors constructed in the same conditions. The maximum currents obtained were 17.41; 18.03 and  $16.50 \text{ } \mu\text{A}$ , whose average value was  $17.30 \text{ } \mu\text{A}$ . Substituting into the straight-line equation,  $308 \text{ } \mu\text{mol L}^{-1}$  is obtained. Thus, the relative error was 2.67 %, considered excellent, since the lake water could contain other interfering substances. Thus, it is verified that the other substances did not interfere with the signal. Figure 5 presents the voltammogram obtained.

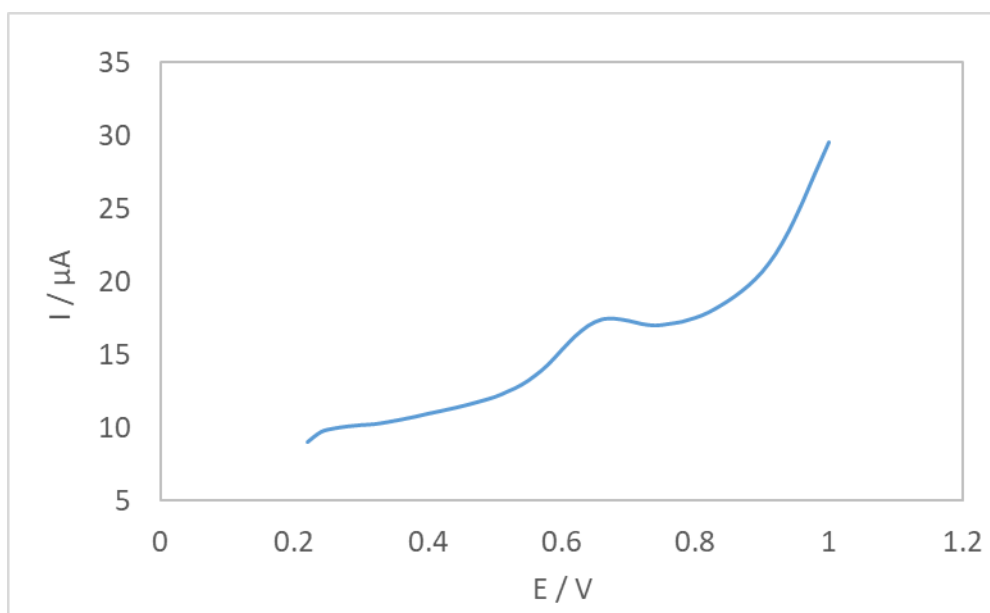

**Figure 5.** Differential Pulse Voltammogram of the sensor in natural water fortified with  $300 \text{ } \mu\text{mol L}^{-1}$  of amoxicillin. Pulse amplitude was 25 mV, at  $50 \text{ mV s}^{-1}$ .